








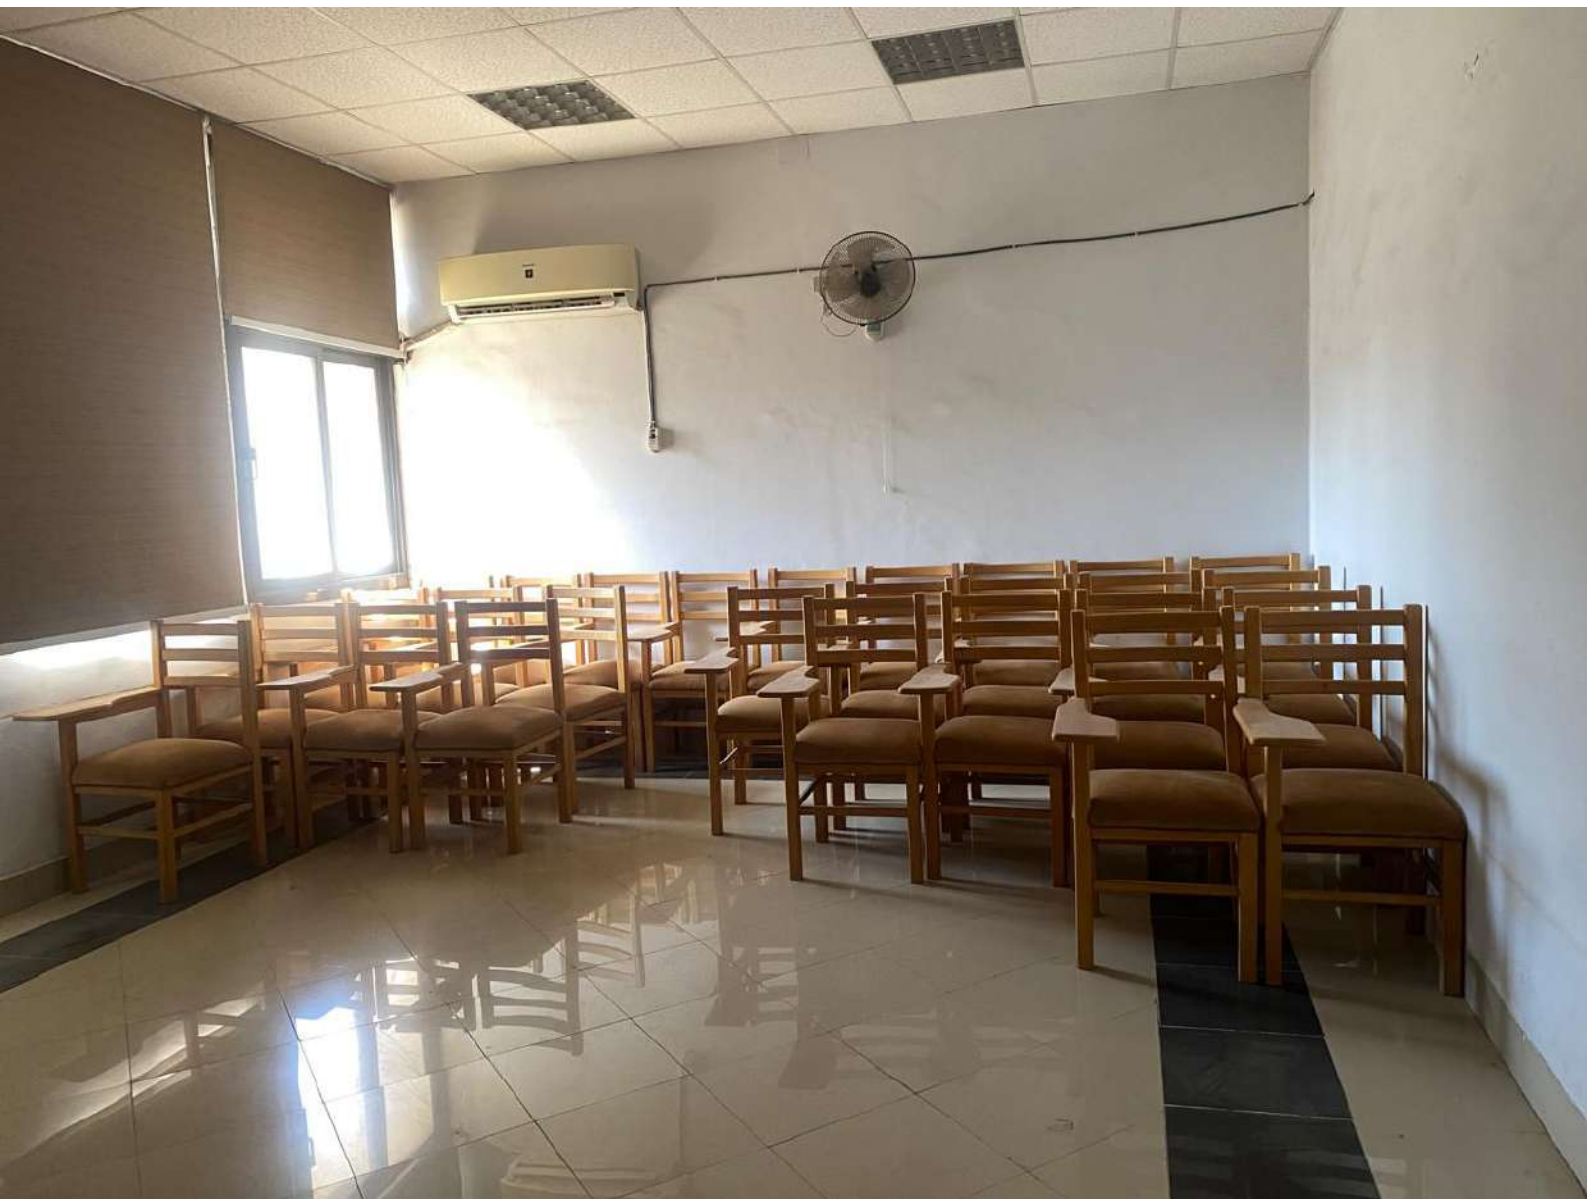

Small white card with text and a blue stamp.





Thermo
SCIENTIFIC



HERACELL VIOS 160i
CO2 incubator

Close regularly
before opening incubator
←
Close



سنترفيوج لفصل الانابيب
الشعريه
Capillary centrifuge



Centrifuge
(max5000rpm)




سنترویفیوچ ١٧

Centrifuge
[max5000rpm]



مشتومينو ج قبره ۱۷

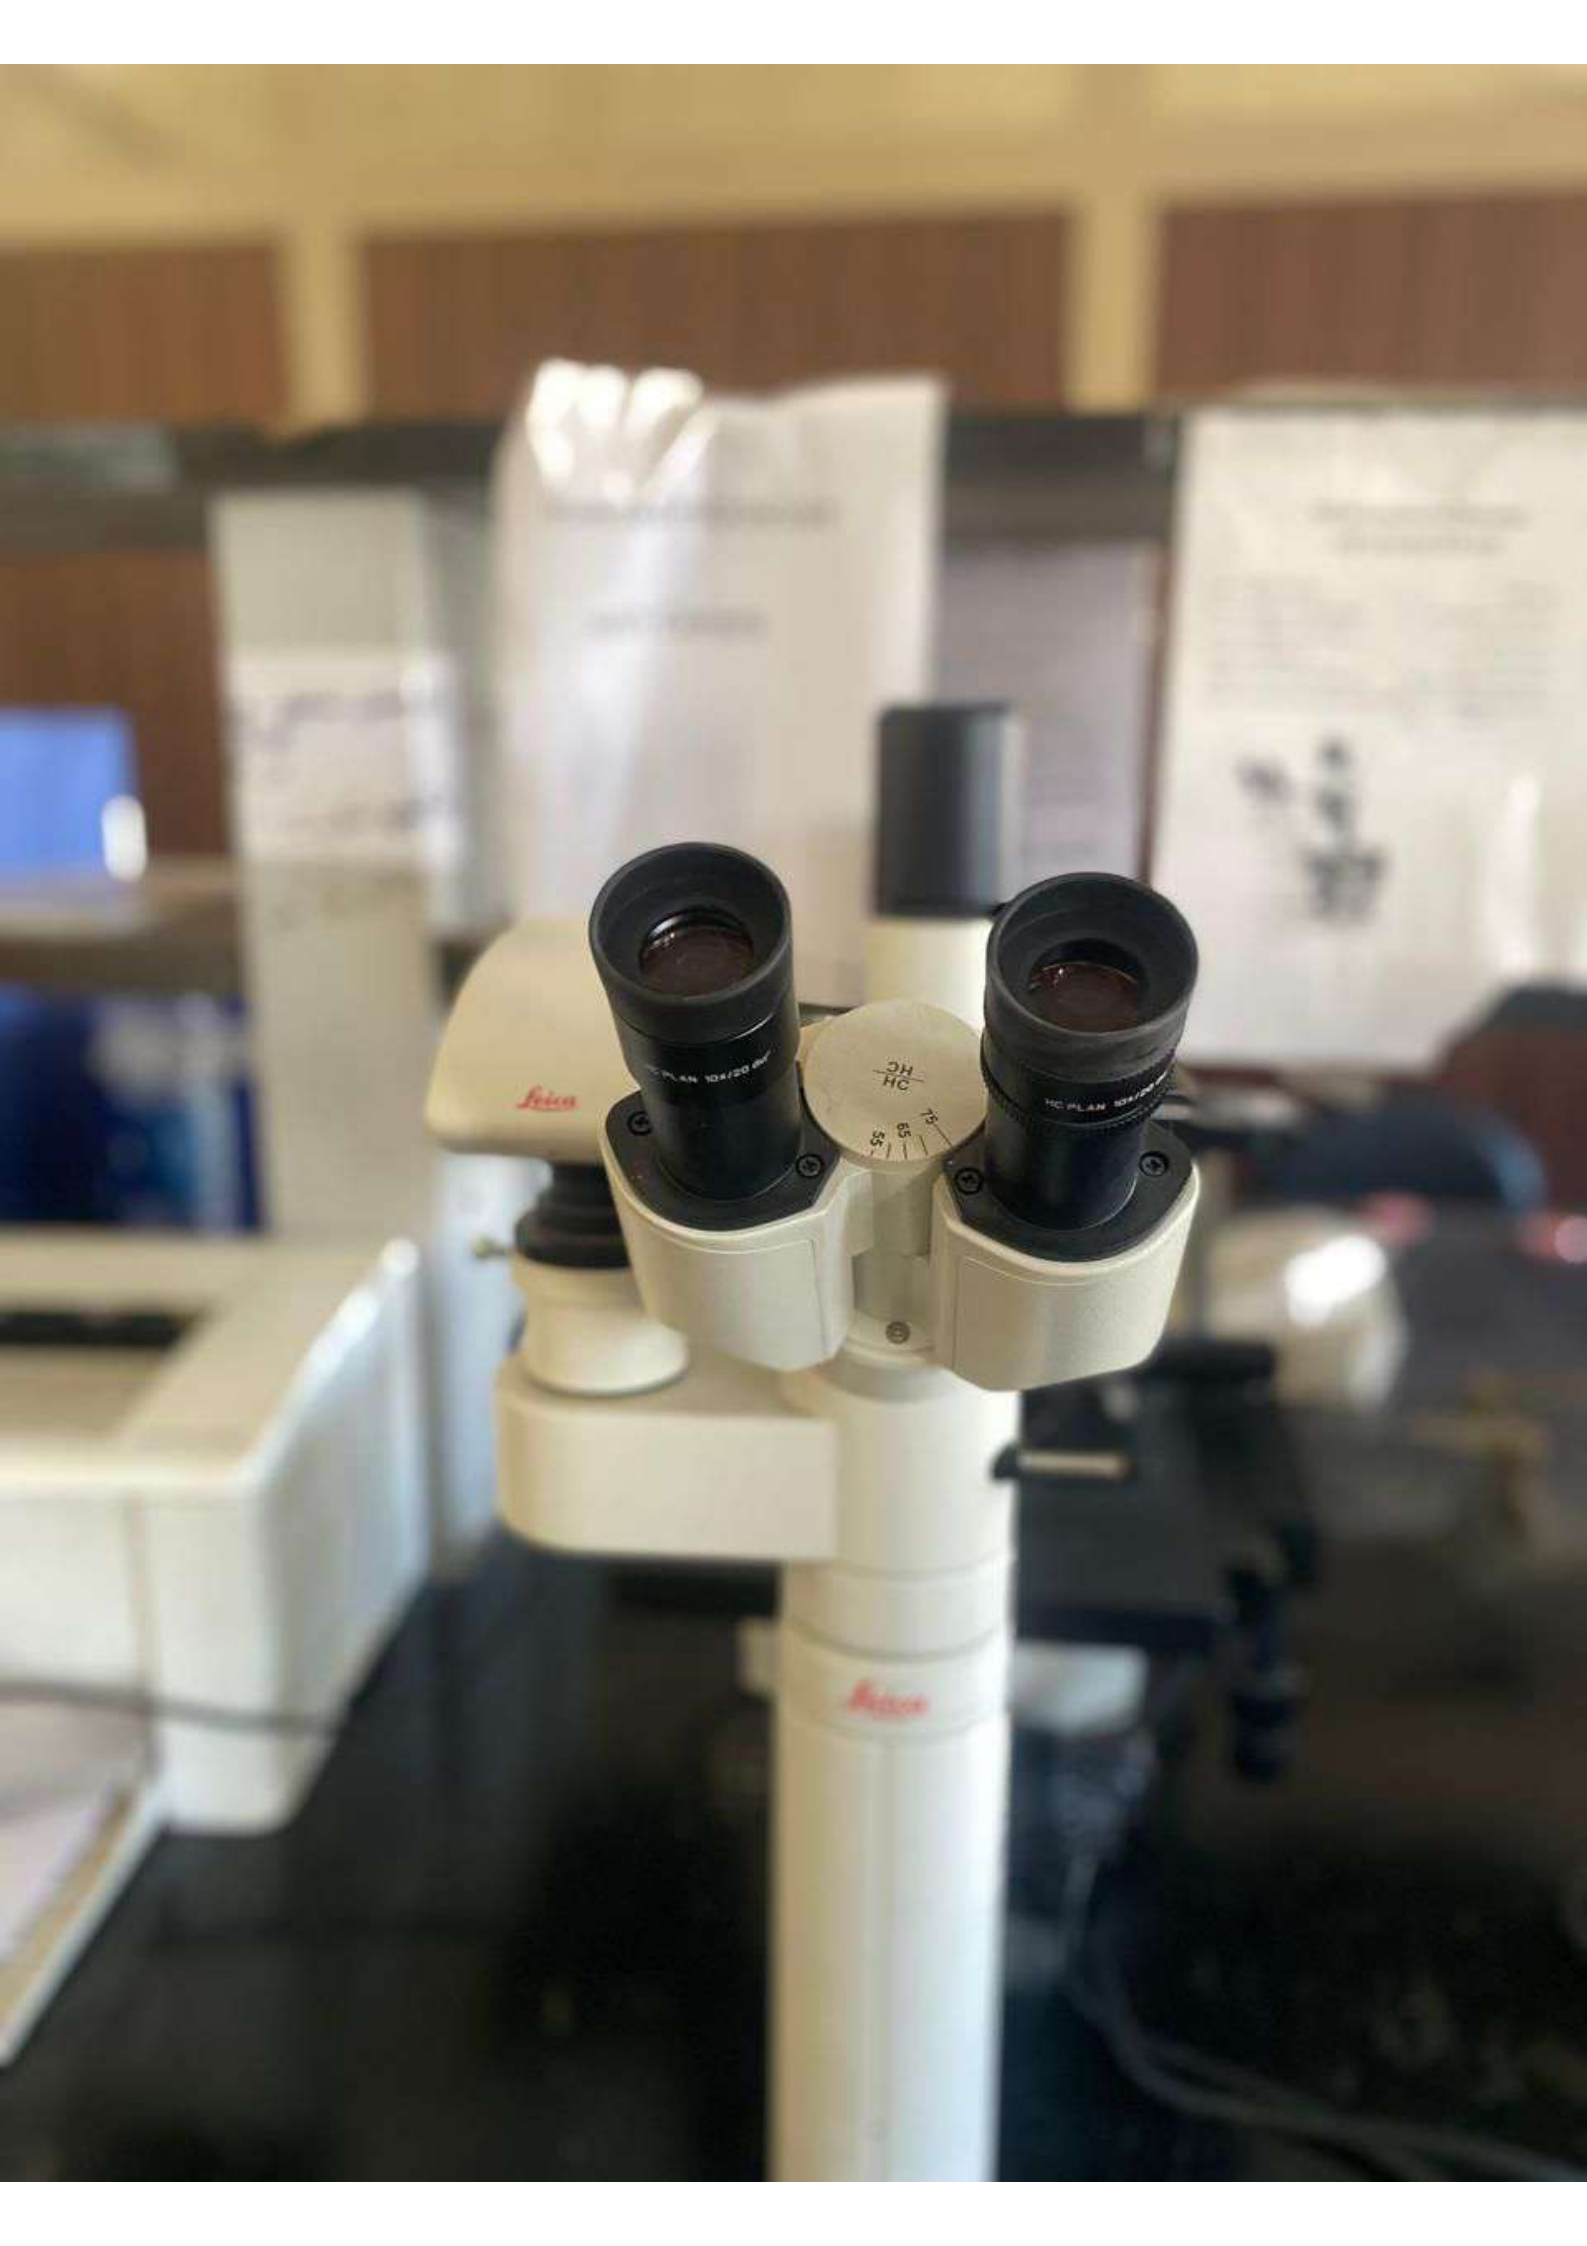

هیم جینیزر

Preparation of 50mM potassium
phosphate buffer pH=7.5

Dissolve 2.2727 g KH_2PO_4 with

5.8002 g of K_2HPO_4

Then the volume was completed to a
liter of distilled water.

تنه خلاصه



سونیکاتور

Soniprep 150

MSE



Power

Time



Timer



Start



Supply



ULTRASONIC CELL CRUSHER NOISE ISOLATING CHAMBER



Intelligent Ultrasonic Processor



Product	Ultrasonic Homogenizer
Model	JY92-IIDN
Ultrasonic Power	900W
Voltage	220V/50Hz
Serial number	C202205432
Taisite Lab Sciences Inc	
Address: 228 Park Ave S 45956, New York, NY 10003, USA	

